



Rysunek nr. 3 - GRUPA 3

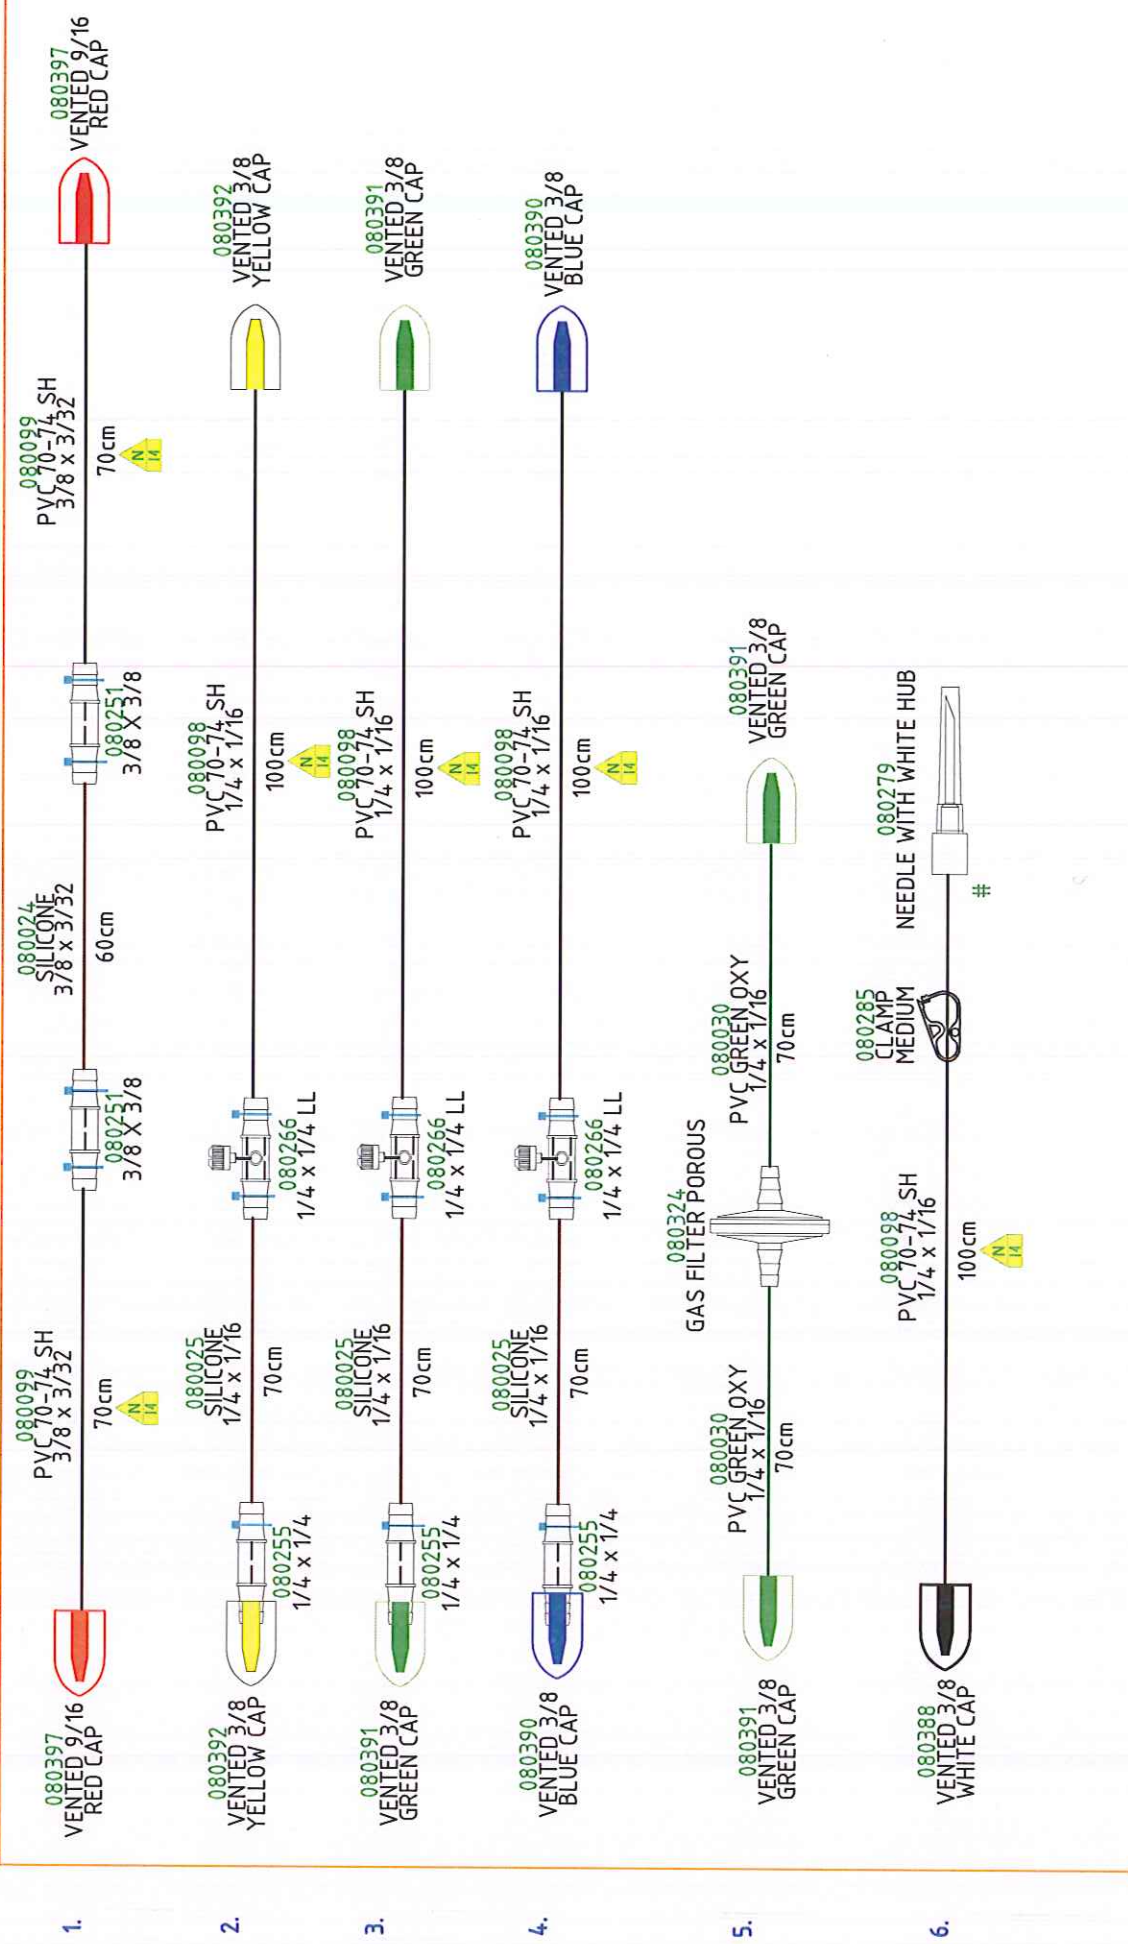

<b>CUSTOMER:</b> CHILDRENS UNIVERSITY HOSPITAL CRACOW POLAND	<b>DESCRIPTION:</b> PAEDIATRIC PACK	<b>DRAWN BY:</b> STEPHEN FLYNN <b>ISSUED:</b> 09/07/2013 <b>INT. AMEND:</b> AMENDED:	<b>ISSUE No:</b> 1 <b>SHEET No:</b> 1/4 THIS DOCUMENT IS THE PROPERTY OF TERUMO EUROPE AND MAY NOT BE COPIED BY ANY THIRD PARTY.
<b>PRODUCT CODE:</b> CX-PL063 <b>ENGINEERING</b>	<b>QUOTATION CODE:</b> XXX	<b>TOTAL PRIME VOLUME:</b>	

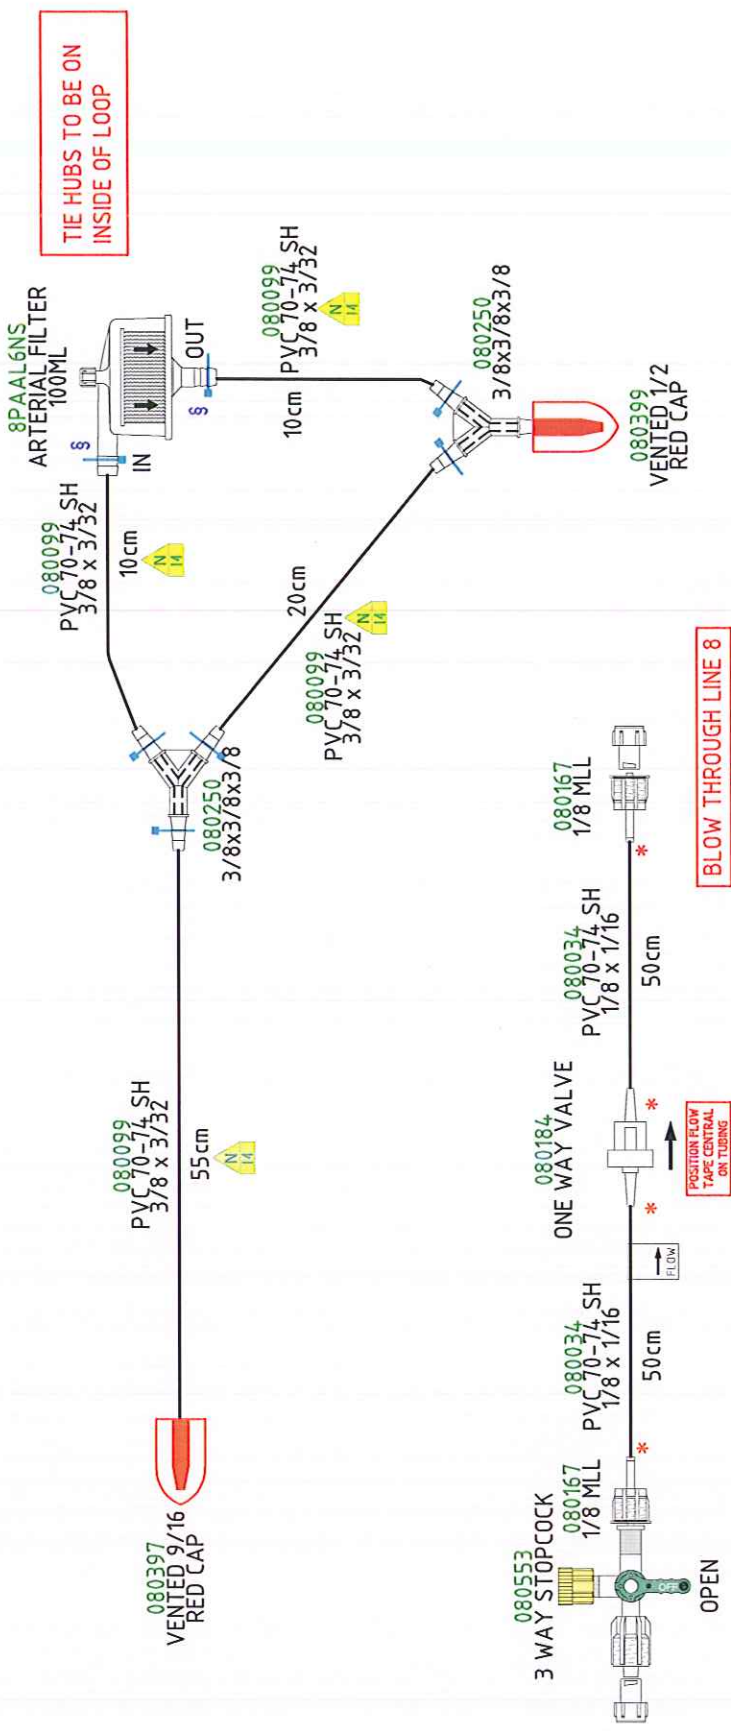

TIE HUBS TO BE ON INSIDE OF LOOP

BLOW THROUGH LINE 8


POSITION FLOW TAPE CENTRAL ON TUBING

7.

8.

<p><b>CUSTOMER:</b> CHILDRENS UNIVERSITY HOSPITAL CRACOW POLAND</p>	<p><b>DESCRIPTION:</b> PAEDIATRIC PACK</p>	<p><b>ISSUED:</b> 09/07/2013 <b>AMENDED:</b></p>	<p><b>ISSUE No:</b> 1 <b>SHEET No:</b> 2/4</p>
<p><b>PRODUCT CODE:</b> CX-PL063</p>	<p><b>QUOTATION CODE:</b> TOTAL PRIME VOLUME: XXX ENGINEERING</p>	<p>THIS DOCUMENT IS THE PROPERTY OF TERUMO EUROPE AND MAY NOT BE COPIED BY ANY THIRD PARTY.</p>	



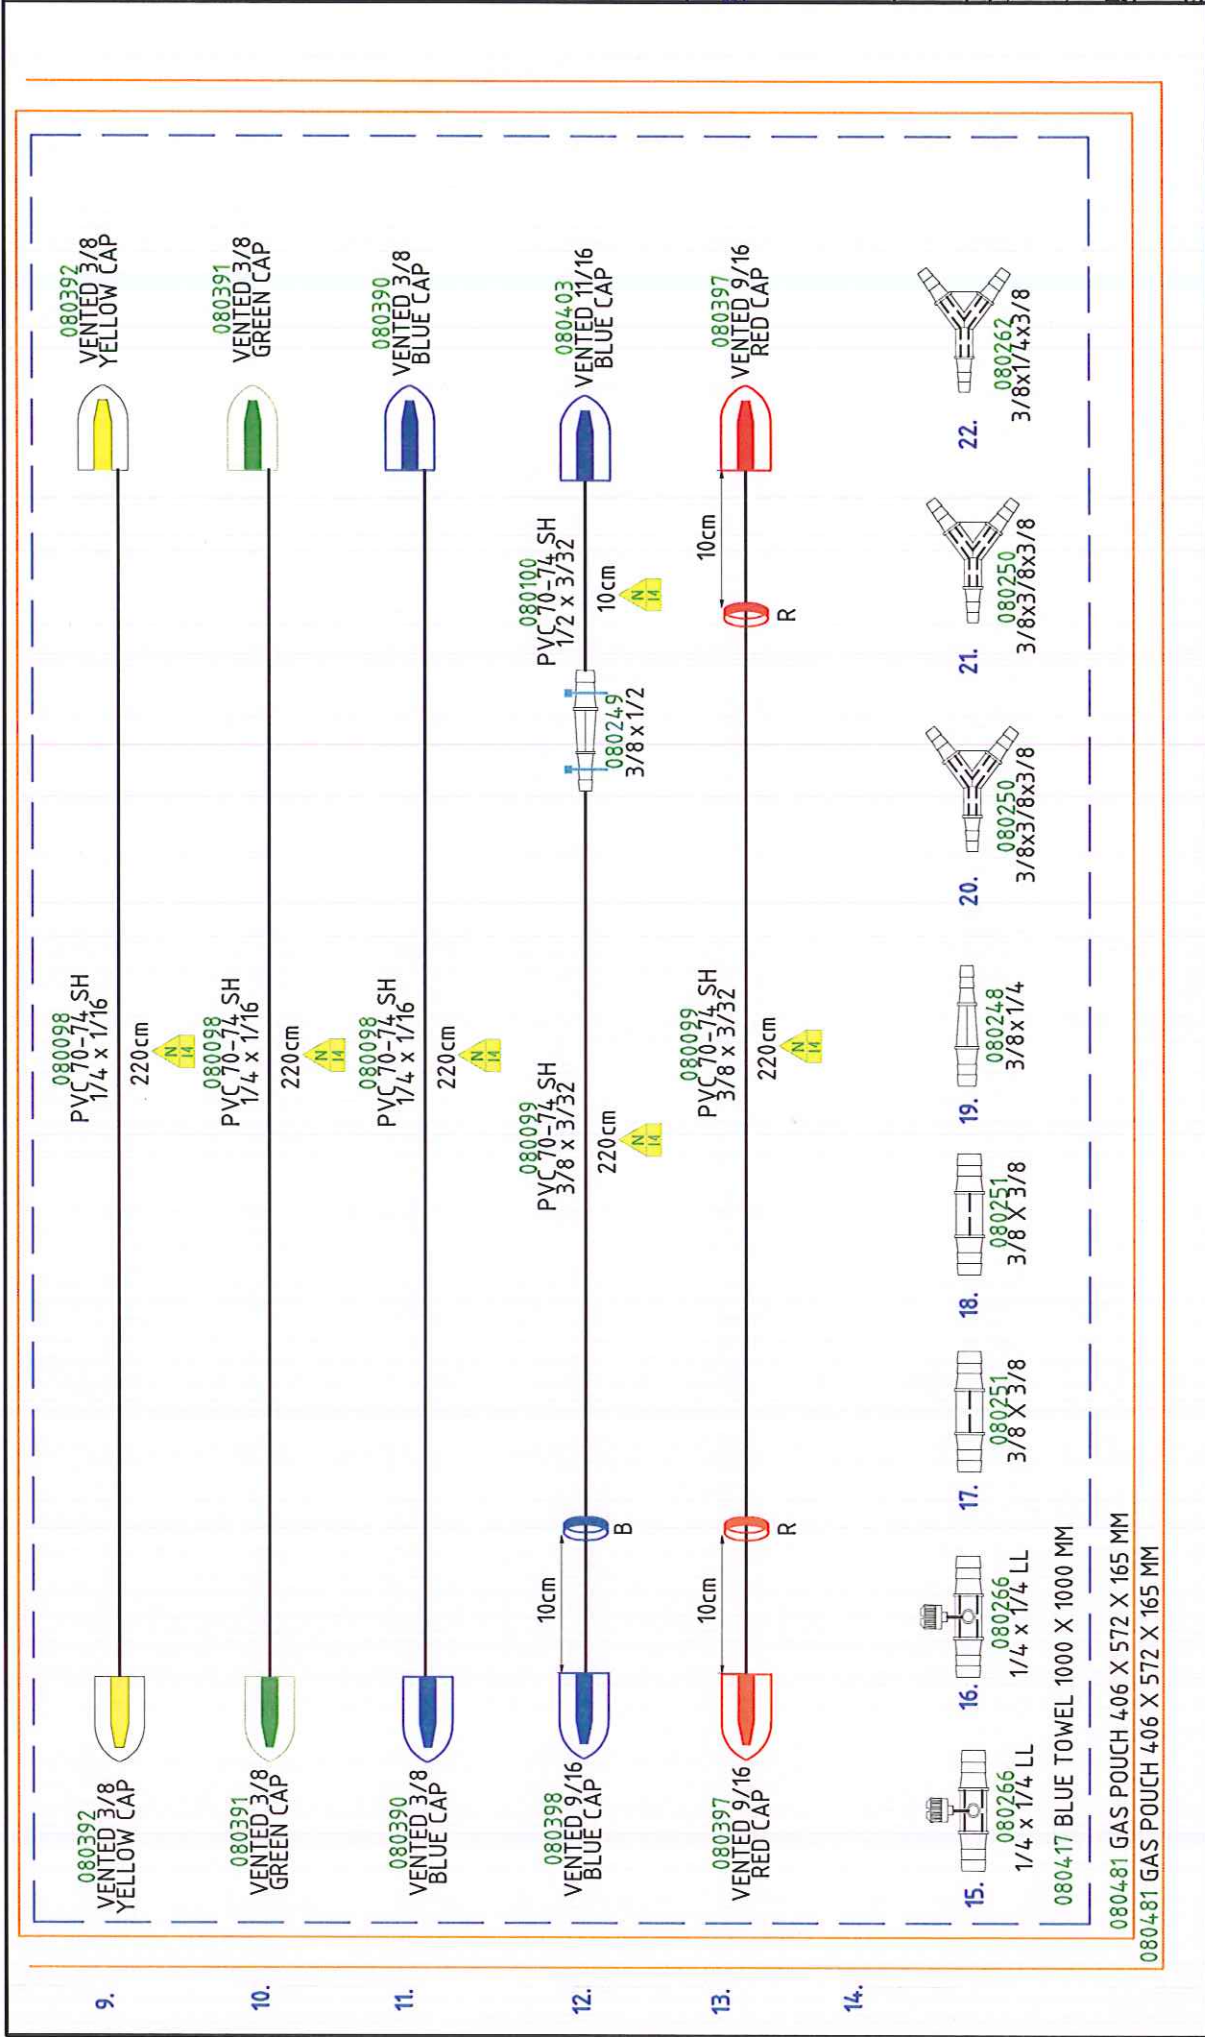

<p><b>CUSTOMER:</b> CHILDRENS UNIVERSITY HOSPITAL CRACOW POLAND</p>	<p><b>DESCRIPTION:</b> PAEDIATRIC PACK</p>	<p><b>PRODUCT CODE:</b> CX-PL063 <b>QUOTATION CODE:</b> ENGINEERING <b>TOTAL PRIME VOLUME:</b> XXX</p>
<p><b>DRAWN BY:</b> STEPHEN FLYNN <b>INT. AMEND:</b></p>	<p><b>ISSUED:</b> 09/07/2013 <b>AMENDED:</b></p>	<p><b>ISSUE No:</b> 1 <b>SHEET No:</b> 3/4 THIS DOCUMENT IS THE PROPERTY OF TERUMO EUROPE AND MAY NOT BE COPIED BY ANY THIRD PARTY.</p>

